


Carbon Accelerator Mass Spectrometry (CAMS) Compact High Throughput

DESIGN

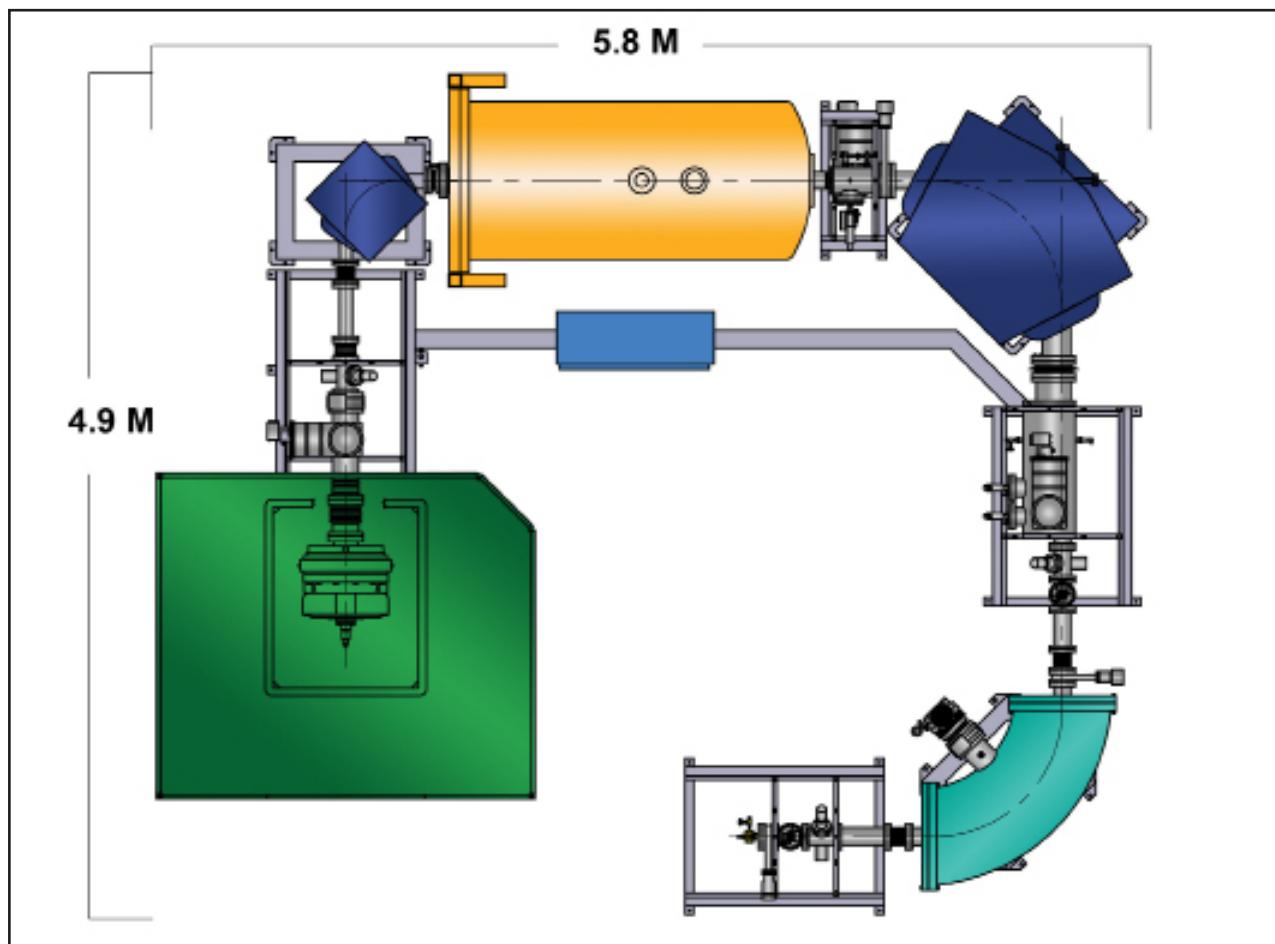

The NEC CAMS is designed for high precision measurement of carbon radioisotope ratios. This is a complete system with all necessary hardware and software for both on-line and off-line radiocarbon isotope ratio measurements.

- Better than 3 per mil precision
- Better than 1×10^{-15} background
- Graphite samples with option for CO₂ samples
- All metal/ceramic acceleration tubes with no organic material in the vacuum volume
- Automated data collection and analysis
- Fully interlocked system designed for unattended operation

ACCELERATOR MASS SPECTROMETRY

AMS is a technique for high precision measurement of radioisotope ratios such as $^{14}\text{C}/^{12}\text{C}$ and $^{14}\text{C}/^{13}\text{C}$. The AMS spectrometer is actually two mass spectrometers in series separated by a molecular dissociator.

The sample is inserted into the ion source at the entrance to the first spectrometer. The sample is converted to negative ions and is accelerated through the spectrometer for a mass separation of better than 1 out of 200. The 90° bending magnet in this spectrometer has a biased chamber to allow sequential injection of the negative ions of interest.

As the negative ions exit the first mass spectrometer, they are accelerated to high potential into a gas stripper to breakup all negative ion molecules and convert the resulting single nuclei ions to positive ions. In this way, such ions as $^{12}\text{CH}^-$, $^{12}\text{CH}_2^-$, $^{13}\text{CH}^-$, and others are converted to single nuclei ions, $^{12}\text{C}^+$, $^{13}\text{C}^+$, and $^{14}\text{C}^+$. These positive ions are then accelerated again to ground potential to the entrance of the second mass spectrometer.

The high energy mass spectrometer is equipped with a 90° dipole bending magnet with a wide exit pole. The abundant isotopes exit this magnet into offset Faraday cups with high precision current integrators. The rare isotope continues on through a 90° electrostatic spherical deflector which removes the low probability events. The final element in the spectrometer is a solid state particle detector.

The entire system is computer controlled for true unattended operation. The CAMS system is designed specifically for carbon radioisotope measurements. Once samples are loaded in the ion source, the system proceeds automatically to switch from sample to sample as the required precisions, time constraints, or other criteria are met. The system can be monitored remotely and is fully interlocked in case of power, water or air failure.




The CAMS system is based on the 500 kV tandem Pelletron accelerator shown in the background, center. This accelerator provides the necessary molecular dissociation while increasing the beam energy to about 1 MeV for the necessary energy dispersion through the second mass spectrometer. This mass spectrometer is shown to the far left. The first mass spectrometer is out of view to the far right. The rare isotope ion beam exits the mass spectrometer into a solid state detector which is in the center foreground.

The mass spectrometer at the high energy end of the tandem Pelletron allows transmission of the rare isotope through the entire system to the particle detector where the ^{14}C events are recorded. The abundant isotopes are stopped in the offset multi Faraday cup chamber immediately following the 90° magnet. The 90° magnet is shown to the far right and the electrostatic deflector is shown in the far left. In the center is the multi Faraday cup chamber which is equipped with high precision current integrators. The entire system is designed with ultrahigh vacuum practices in mind.



MULTI-SAMPLE NEGATIVE ION SOURCE

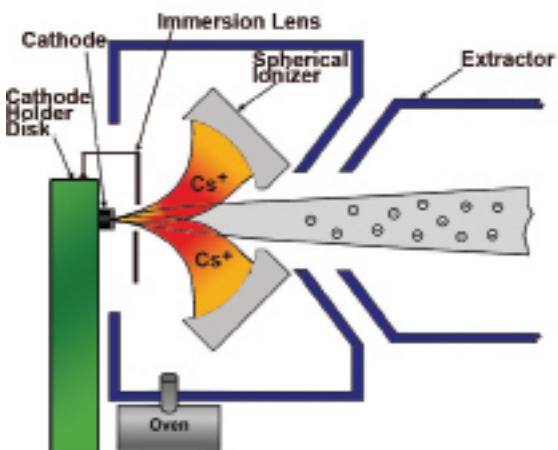

For carbon AMS the sample is either graphite or carbon dioxide. In both cases, the sample is contained in a cathode holder. In the case of carbon dioxide, the gas flows through this cathode holder. Cesium vapor is in the area of the cathode holder which coats the cooled cathode with a thin layer of cesium while cesium is also ionized forming a cesium beam which strikes the AMS sample material. The sputtered particles are converted to negative ions by passing through the cesium layer. The resultant negative ion beam is extracted for acceleration through the mass spectrometer.


The cathode holders are mounted on a removable cathode disk. There is a valve assembly which allows the removal of the cathode disk without disturbing the cesiated volume.

AMS CONTROL SYSTEM

The NEC AMS control system monitors and controls all AMS parameters. The vacuum system is fully interlocked and hardwired to be independent of the computer control system. However, the control system does monitor all vacuum parameters.

The control system hardware is based on CAMAC protocols. The control system software is based on Scientific Linux with X Windows and the NEC AccelNET system. The overall control system is designed for fully automated sample running by events, precision or time. All parameters can be saved and restored for easy start up. The system is designed for true remote operation via web interface which allows direct diagnostics from the NEC factory for rapid customer support.

System start up and ion beam tuning is made easy by assignable knobs and analog meters. The software is equipped with flat topping routines, energy and mass determination through the bending magnets, software strip chart recorders, and storage of all AMS parameters for every ^{14}C event.

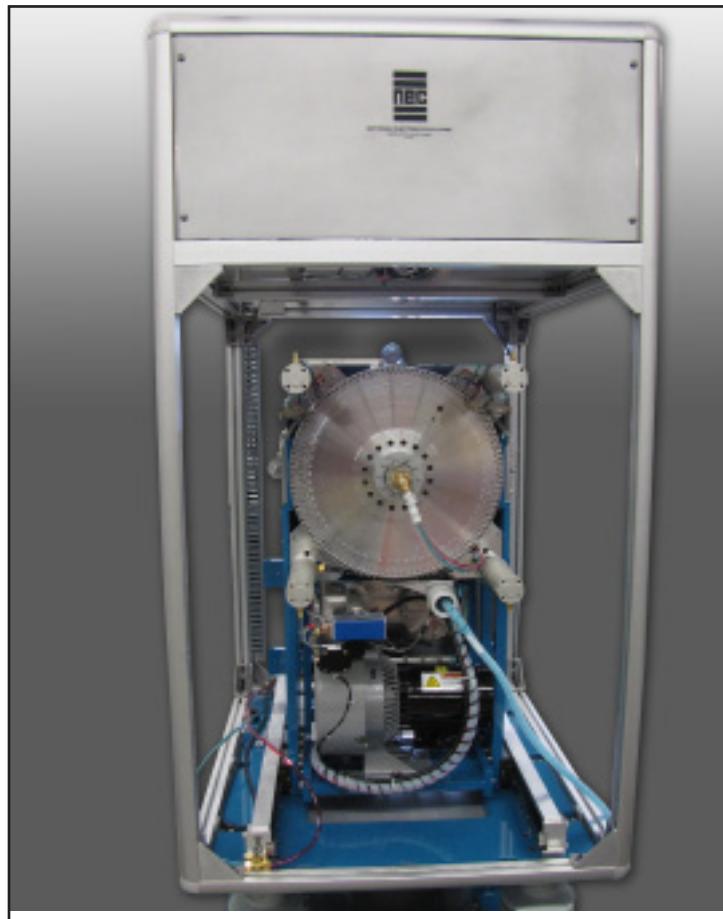

The NEC 134 sample Multi-Cathode Source of Negative Ions by Cesium Sputtering (MC-SNICS) is designed for high throughput applications where a large number of AMS samples is expected in a short period of time. The 134 MC-SNICS is equipped with bi-directional cathode indexing for rapid location of any cathode in any of the 134 positions. The simple cathode indexing system has proven to be highly reliable and is fully computer controlled to allow the analysis of groups of AMS samples in any order.



PERFORMANCE SPECIFICATIONS FOR THE NEC COMPACT, CARBON AMS SYSTEM

PELLETRON SPECIFICATIONS

Insulating Column Voltage Rating	0.6 Megavolts
Voltage Stability	Better than 1 kV
Voltage Ripple	<=500 V FWHM as measured by CPO at 0.5 MV Terminal Voltage
Singly Charged Ion Energy Range	to 1.0 MeV
Charging Current Rating	100 microamps (60 Hz Power) 83 microamps (50 Hz Power)
Acceptance Test Values	
$^{13}\text{C}^+$	0.3 microamps peak pulsed current at 0.5 MV terminal voltage

AMS MEASUREMENTS

Ratio of $^{14}\text{C}/^{13}\text{C}$ from measurements of three (3) "modern" graphite carbon samples with a precision of 0.3% or better, using known solid samples of unlimited size provided by the buyer.

Ratio of $^{13}\text{C}/^{12}\text{C}$ from three (3) solid graphite samples of unlimited size 0.3% or better.

Ratio of $^{14}\text{C}/^{12}\text{C}$ from three (3) dead graphite samples of unlimited size 2×10^{-15} or lower using Alfa Aesar graphite supplied by NEC.

[CAMS]



7540 Graber Rd., P.O. Box 620310,
Middleton, WI 53562-0310 USA
TELEPHONE: 608-831-7600 ♦ **FAX:** 608-831-9591
E-MAIL: nec@pelletron.com ♦ **WEB-SITE:** <http://www.pelletron.com>